



A case study: The deployment of a novel *in situ* fluorimeter for monitoring biological contamination within the urban surface waters of Kolkata, India



B.G. Fox^a, R.M.S. Thorn^a, T.K. Dutta^b, M.J. Bowes^c, D.S. Read^c, D.M. Reynolds^{a,*}

^a Centre for Research in Biosciences, University of the West of England (UWE), Bristol, Frenchay Campus, Bristol BS16 1QY, UK


^b Department of Microbiology, Bose Institute P-1/12 C.I.T. Scheme VII-M, Centenary Campus, Kolkata 700054, India

^c UK Centre for Ecology & Hydrology (UKCEH), Benson Lane, Crowmarsh Gifford, Wallingford OX10 8BB, UK

HIGHLIGHTS

- Better water quality monitoring requires more appropriate water quality parameters.
- Peak T fluorescence could be used to monitor microbial activity in aquatic systems.
- *In situ* Peak T fluorimeter was deployed in urban surface waters in Kolkata.
- Fluorimeter response was compared to other traditional water quality analyses.
- Sensor able to detect biological pollution in real-time in freshwater systems.

GRAPHICAL ABSTRACT

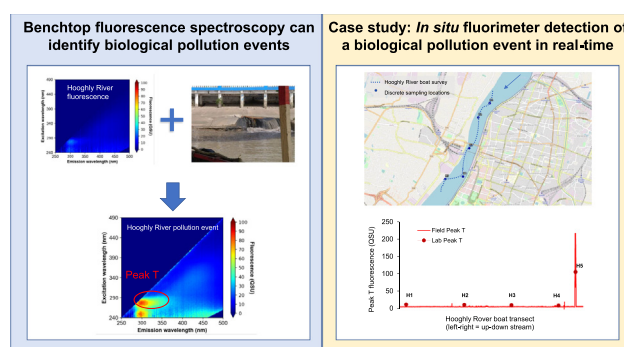

ARTICLE INFO

Editor: Warish Ahmed

Keywords:

Biological contamination
Fluorescent organic matter
Freshwater
Surface waters
In situ sensors
Water quality

ABSTRACT

The quality and health of many of our vital freshwater systems are poor. To tackle this with ever increasing pressures from anthropogenic and climatic changes, we must improve water quality monitoring and devise and implement more appropriate water quality parameters. Recent research has highlighted the potential for Peak T fluorescence (tryptophan-like fluorescence, TLF) to monitor microbial activity in aquatic systems. The VLux TPro (Chelsea Technologies Ltd., UK), an *in situ* real-time fluorimeter, was deployed in different urban freshwater bodies within Kolkata (West Bengal, India) during March 2019. This study is the first to apply this technology in surface waters within a densely populated urban area. Spot-sampling was also undertaken at 13 sampling locations enabling physicochemical analysis, bacterial enumeration and determination of nutrient (nitrate and phosphate) concentrations. This case study has demonstrated the ability of an *in situ* fluorimeter, VLux TPro, to successfully identify both biological contamination events and potential elevated microbial activity, related to nutrient loading, in complex surface freshwaters, without the need for expensive and time-consuming laboratory analysis.

1. Introduction

Monitoring water quality globally is considered vital for human health and sustainable development, as well as ensuring aquatic ecosystem integrity (Firth, 1999; Postel, 2015). With increasing pressures on water sources due to population growth, industrialisation, agriculture, urbanisation and

climatic changes (Khamis et al., 2017; Patil et al., 2012), it has become essential to manage our water sources effectively. To do this, we must be able to successfully monitor water quality with good spatio-temporal resolution (Postel, 2015).

The most frequently and routinely measured water quality parameters are physicochemical, chemical and biological in nature which rely on discrete sampling and lengthy, as well as expensive, laboratory testing (Blaen et al., 2016; Peleato et al., 2017). The measurement of such water quality parameters provides information relating to the structure of the

* Corresponding author.

E-mail address: Darren.Reynolds@uwe.ac.uk (D.M. Reynolds).

aquatic ecosystem under investigation but does not provide information that usefully relate to the function of the monitored ecosystem (Matilainen et al., 2011; Patil et al., 2012). In particular, the routine measurement of the biological qualities of freshwater systems is performed by the measurement of biological indices that require macro-biological diversity assessment (surveys) and microbiological analysis via the culturing of specific indicator species (Bio-Science Division and Central Pollution Control Board, 2018; Central Pollution Control Board, 2017). The reliance on discrete sampling and laboratory testing limits the response needed to manage catchments that experience rapidly changing dynamic ecosystem interactions.

The formation of the Central Pollution Control Board in India has greatly benefitted the monitoring of Indian river systems at a catchment scale, providing a holistic approach to water quality assessment. Under the national water quality monitoring programme there are 9 core parameters monitored monthly: pH, temperature, conductivity, dissolved oxygen, BOD, nitrate, nitrite, faecal coliforms and total coliforms (Central Pollution Control Board, 2013). Alongside these core parameters, location-specific studies collect data for a range of field-based observations, general parameters, trace metals and pesticides (Central Pollution Control Board, 2013). Biological water quality data is related to three parameters: saprobity index, a quantitative inventory of the presence of macro-invertebrate benthic fauna; diversity index, the evaluation of benthic fauna using the same animals collected for the estimation of the saprobic score; and production-respiration (P/R) ratio, ratio of gross production to total community respiration (Bio-Science Division and Central Pollution Control Board, 2018; Central Pollution Control Board, 2017, Central Pollution Control Board, 2013). However, the latter parameter is infrequently used with biological water quality classification, commonly determined by combining the saprobic and diversity scores (Bio-Science Division and Central Pollution Control Board, 2018; Central Pollution Control Board, 2017).

Although improvements have been made, the assessment of these biological indices in freshwater biomes is still difficult to quantify with current approaches and practices. Furthermore, very little information or data is collected in real-time with biotic indices informing longer-term environmental conditions (Aazami et al., 2015; Santos et al., 2021). Whilst important to understand, the reliance on long-term biological changes for the assessment of pollution levels makes it difficult to implement timely intervention strategies especially within large and dynamic riverine systems (Santos et al., 2021). To combat this issue, there is the need to develop new monitoring parameters which enhance our understanding of water quality dynamics and processes, that take advantage of technological developments and real-time acquisition. Real-time technologies provide advantages in terms of streamlining the data collection process, reducing cost in the long-term and, critically, producing higher resolution data (Chowdury et al., 2019).

Water quality sensors are widely available for the monitoring of basic physicochemical parameters, but these sensors do not yet provide information regarding biotic parameters or biological processes that take place within aquatic systems. Fluorescence-based sensing technology has long been utilised for the identification of anthropogenic pollutants, such as polycyclic aromatic hydrocarbons (PAH) and optical brighteners (Cyr et al., 2019). Recently *in situ* real-time portable fluorimeters have been developed for sensing biological contamination. Research concerning aquatic fluorescent organic matter (AFOM) has highlighted the potential of tryptophan-like fluorescence (TLF or Peak T; $\lambda_{ex}/\lambda_{em}$ 275/340–360 nm) for tracing microbial contamination events (Blaen et al., 2016; Carstea et al., 2020; Coble et al., 2014; Fox et al., 2017; Hudson et al., 2008; Sorensen et al., 2018b; Sorensen et al., 2021, Sorensen et al., 2015b; Zhou et al., 2017). The widespread use of this technology for monitoring water quality has been limited by the inability to disentangle optical interferences caused by scattering (turbidity) and absorption (excess inorganic and organic material) (Khamis et al., 2015; Mendoza et al., 2020). Such optical interferences obviate the reporting of fluorescence in standardised units of measurements thus preventing the comparison of quantitative data for different aquatic sites. In this study we investigate if real-time

Peak T values from an *in situ* fluorimeter (VLux TPro, Chelsea Technologies Ltd.), corrected for absorbance and turbidity, can be used to infer bacterial and nutrient contamination. The aim of this work is to deploy the VLux TPro for the first time to provide quantitative assessments of the biological properties of urban surface waters present in the densely populated city of Kolkata. This research reports the identification of wastewater contamination events from point sources. The benefit of utilising Peak T fluorescence to directly measure the “biological activity” in aquatic environments is demonstrated and the use of this new water quality information to inform biological contamination events in complex surface water matrices is discussed.

2. Materials and method

2.1. Study area

All field sites were located within the city of Kolkata, in the state of West Bengal, India. Kolkata has undergone various stages of expansion and urbanisation over the past 300 years, turning this marshland into a booming trading port, and now into a megacity (Bhattacharjee, 2014; Gangopadhyay and Patra, 2019). At the last census in 2011, Kolkata city (an area of 185 km²) had a population of almost five million people, with over 14 million living in the Kolkata Metropolitan Area (1851.41 km²) (Bhattacharjee, 2014). The large population, thriving industry, and sustained and often unregulated urbanisation continues to put pressure on the water resources in Kolkata (Gangopadhyay and Patra, 2019; Gangopadhyay and Gupta, 2008). The field sampling locations were classified into sample types based on water course type: (1) The Hooghly River (Ganga); (2) Canals; (3) East Kolkata Wetlands.

The Hooghly River is a distributary of the Ganges River, and often referred to locally as the Ganga (Central Pollution Control Board, 2013; Gangopadhyay and Patra, 2019). It is of great cultural and social significance within India, being used for bathing and religious ceremonies and celebrations (Bio-Science Division and Central Pollution Control Board, 2018). It is also used as a shipping channel for goods boats and passenger ferries alike. This watercourse is subject to a range of pollution sources (Bio-Science Division and Central Pollution Control Board, 2018), receiving wastewater from 22 polluting industries within West Bengal, with the point sources in Kolkata contributing to 74 % of this loading (Central Pollution Control Board, 2013). The water quality of the Hooghly River in Kolkata is classified as Class D (heavy pollution), although the biological water quality, based on saprobic and diversity score, of the Hooghly in Kolkata is classified as moderately polluted (Class C) (Bio-Science Division and Central Pollution Control Board, 2018). The Ganga Action Plan (GAP) aims to improve this to bathing water quality (Class B) (National River Conservation Directorate, 2009).

The canal system in Kolkata originated from channels used for local transport and trade, as well as an irrigation source (Gangopadhyay and Patra, 2019). As the city expanded, the canal system was also expanded to accommodate increased trade within the city and to transport goods beyond Kolkata (Bhattacharjee, 2014; Gangopadhyay and Patra, 2019). Over time, the canals began to deteriorate, mainly due to sedimentation, leading to a decline in their use. Some of the canals were repurposed to redirect storm water and sewage from east of the old city, into the River Bidvadhari. Many canals ceased to be used for transport or trade and were scarcely maintained (Bhattacharjee, 2014), effectively turning them in drainage channels for storm waters and sewage (Gangopadhyay and Patra, 2019; Gangopadhyay and Gupta, 2008).

The East Kolkata Wetlands (EKW) are host to the world's largest sewage fed aquaculture system (EKWMA, 2016). Originally, these wetlands existed as fisheries to the east of the city and later as the location for diverted storm waters and sewage (Bhattacharjee, 2014; EKWMA, 2016). At present, the EKW not only act as the only sewage treatment for a third of the city's sewage, via filtration, sediment settlement and nutrient acquisition, but also provide food and a livelihood for many of the local population (Central Pollution Control Board, 2020; East Kolkata Wetlands Management

Authority, 2019). To protect the area from rapid expansion, they were marked as a Ramsar site in 2002 and designated as one of the “Wetlands of International Importance” (EKWMA, 2016). The wetland ponds are surrounded by a network of small channels which are fed from the canal network, in particular Circular Canal (Bhattacharjee, 2014; Gangopadhyay and Patra, 2019).

2.2. Sampling survey

The data presented in this case study was collected during a sampling survey which took place between 11th – 26th March 2019, prior to the monsoon (which usually begins at the start of June) and to avoid peak annual temperatures. The modelled average monthly flow rate for the Hooghly River in Kolkata throughout 2019 ranged from 20.27 to 937.83 m³/s, with the lowest flow occurring in March and the highest in August (Sutanudjaja et al., 2018). The sampling survey analysed a total of 13 sampling sites, seven were located on the Hooghly River, four from the canal network and two samples from the East Kolkata Wetlands (EKW). A single sample was collected from each of the 13 sample sites. The locations for all sampling sites monitored are shown in Fig. 1, and a table of all sampling location details (from GPS data) can be found in Supplementary Table 1.

2.2.1. Collection of water samples

Water samples were collected from the centre of the water body where possible, or alternatively at margin locations with visual evidence of flow, to ensure mixing (Bowes et al., 2020). Samples were collected using a 500 mL PTFE bottle, rinsed with the sample three times prior to collection. The collection bottle was deployed to a depth of 30 cm, then decanted, unfiltered, into two 50 mL sterile falcon tubes, one 60 mL acid-washed (20 % hydrochloric acid) Nalgene PTFE bottle, and two sterile 1.5 mL microcentrifuge tubes. One microcentrifuge tube was pre-prepared with glutaraldehyde, with a final concentration of 0.25 %, to act as a fixative for storage. Subsequently, two 60 mL acid washed PTFE bottles were filled with a filtered subsample (0.45 µm sterile ThermoFisher cellulose nitrate

membrane filters). All samples were kept in the dark and at 4 °C when stored and kept chilled during transport.

2.2.2. Physicochemical parameters

The following key physicochemical parameters were measured in the field; dissolved oxygen (DO), electrical conductivity (hereby referred to as conductivity), temperature and pH. DO was measured immediately after sample collection using a handheld meter (HQ10, Hach, CO, USA). Conductivity and temperature data were collected using a handheld Accumet™ conductivity meter (Fisherbrand, Pittsburgh, USA), and pH was measured with a handheld pH meter (Jenway 570, Cole-Parmer, Illinois, USA).

2.2.3. VLux TPro sensor

Field trials were conducted using a prototype of the VLux TPro optical sensor (Chelsea Technologies Ltd., UK) for measuring fluorescence intensity of Peak T, Peak C and chlorophyll- α , as well as absorbance and turbidity (Fox, 2018). All fluorescence data is measured at an excitation wavelength of 280 nm, with Peak T, Peak C and chlorophyll- α fluorescence emission measured at 365 ± 25 nm, 450 ± 25 nm and 682 ± 15 nm respectively. The sensor has a dynamic range of 0–600 quinine sulphate units (QSU) and sensitivity of 0.02 QSU for the fluorescence channels. Absorbance was also measured at an excitation wavelength of 280 nm, with a dynamic range of 0–3.5 optical density (OD) and sensitivity of 0.002 OD. The turbidity channel measured at an excitation and emission wavelength of 860 nm, in line with ISO 7027:1999(E) (ISO, 1999), and has a dynamic range of 0–1000 Formazin Nephelometric Units (FNU) and sensitivity of 0.01 FNU (Fox, 2018). All VLux TPro fluorescence sensing data output is corrected for optical interferences using real-time and *in situ* absorbance and turbidity measurements. All corrections are applied through internal software algorithms, reporting all fluorescence measurements in quinine sulphate units (QSU). A QSU value of 1 is equivalent to 1 ppb of quinine sulphate standard in 0.1 M perchloric acid (Starna Cells, USA) at $\lambda_{ex}/\lambda_{em}$ 347.5/450 nm (Fox, 2018).

The VLux TPro was deployed to a depth of 30 cm at all monitoring sites, as per collected water samples. Data collected was logged using a custom-made data logger, using a Raspberry Pi 3 B+ (The Raspberry Pie

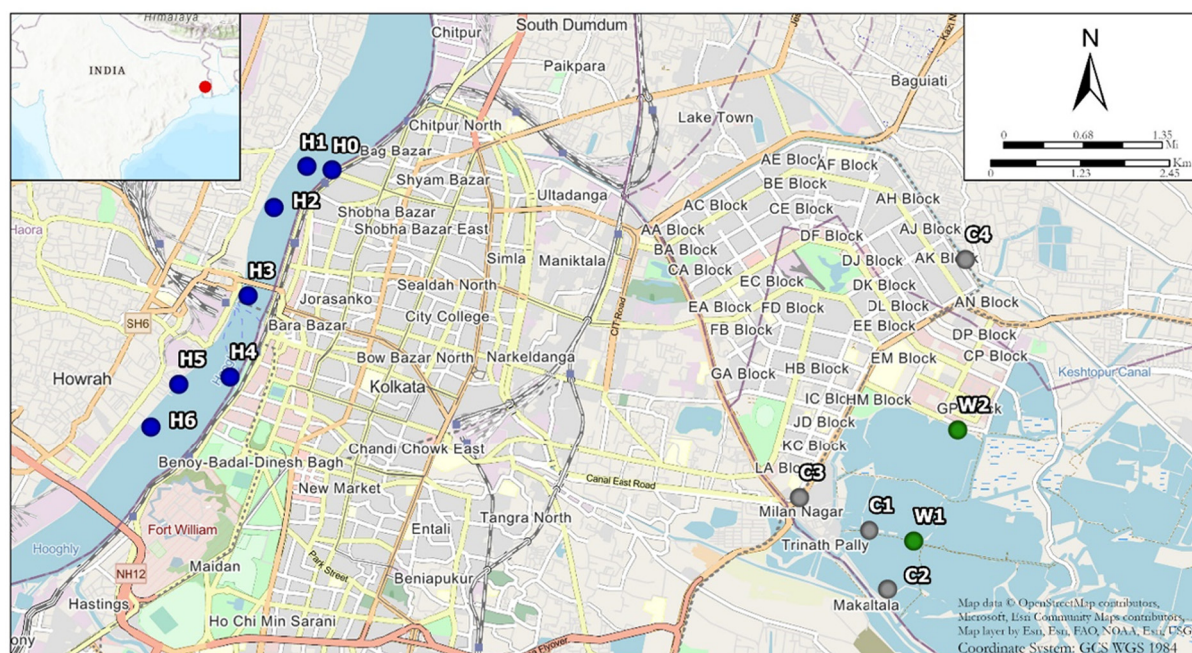


Fig. 1. Study site map of sampling locations in urban Kolkata for the sampling survey conducted in March 2019. All field locations are labelled and identified using a coloured marker: Hooghly River [Hx] = blue; canal locations [Cx] = grey; and, East Kolkata Wetlands (EKW) [Wx] = green. An overview map is provided in the top left and scale information detailed in the top right. Map created in ArcGIS® Pro (ESRI™, California, US) using OpenStreetMap data (2021).

Foundation, UK) in conjunction with a custom logging general user interface (GUI) created in Python™ (Python Software Foundation).

2.3. Laboratory analysis of water samples

2.3.1. Microbiological analysis

Microbiological analysis for *Escherichia coli* and coliform enumeration was undertaken within 6 h of sample collection. A standard dilution series using sterilised de-ionised water was prepared and each dilution filtered onto a sterile 0.2 µm membrane filter (Whatman® 0.2 µm nitrocellulose membrane filters, GE Healthcare, UK), and placed on Membrane Lactose Glucuronide Agar (MLGA) plates, as per the coliform membrane filtration method (Sartory and Howard, 1992; The Environment Agency, 2008). This method allows for *Escherichia coli* and coliforms to be differentiated and enumerated.

Analysis for total bacteria cell count was conducted via flow cytometry, using a Gallios flow cytometer (Beckman-Coulter, UK). An aliquot of 0.5 mL from each glutaraldehyde fixed sample was stained with SYBR Green I (Sigma-Aldrich, UK) at a final concentration of 1:1000 for 30 min at room temperature in the dark. An addition of 2.0 µL of 1 µm diameter beads (Life Technologies, UK) to each sample was used as a calibration and counting standard. Each sample was run for 1 min at a low flow rate using excitation with a 488 nm laser. Gates were manually drawn in Kaluza 1.2 software (Beckman-Coulter, UK) to distinguish and count bacterial cells from background noise and non-bacterial particles.

2.3.2. Nutrient analysis

Samples were analysed for nutrient concentrations at the UK Centre for Ecology & Hydrology (UKCEH). All analyses were carried out immediately on return to the UK, which was between 2 and 18 days after sample collection. Concentrations for total phosphorus, total dissolved phosphorus, soluble reactive phosphorus, and dissolved ammonium were determined as described by Bowes et al. (2020). Dissolved organic carbon (DOC) was analysed by thermal oxidation using an Elementar Vario Cube (Elementar Analysensysteme GmbH, Germany) (Bowes et al., 2020). Major dissolved anion concentrations (fluoride, chloride, nitrite, nitrate and sulphate) were determined using ion chromatography (Dionex AS50, Thermo Fisher Scientific, USA) (Bowes et al., 2020). Aquacheck quality control standards (LGC Standards, UK) were used for all analyses.

Table 1

Physicochemical and chemical water quality data, and optical data (from the VLux TPro sensor) for the Hooghly River, Canal and the East Kolkata Wetland (EKW) water samples. Data shown is the parameter average for each water type ± 1 standard deviation: six field sites on the Hooghly River; four canal water field sites; and two field sites in the East Kolkata Wetlands (EKW).

	Hooghly	Canals	EKW
Physicochemical data			
DO (mg/L)	5.375 \pm 0.392	1.135 \pm 0.589	13.285 \pm 3.174
pH	7.982 \pm 0.074	7.160 \pm 0.492	8.950 \pm 0.381
Conductivity (µS/cm)	343.017 \pm 19.854	1192.650 \pm 303.249	788.500 \pm 36.062
Temperature (°C)	29.37 \pm 1.61	28.875 \pm 0.767	31.000 \pm 1.556
Chemical data			
Soluble reactive phosphorus (mg/L)	0.005 \pm 0.003	0.834 \pm 0.581	0.010 \pm 0.057
Total phosphorus (mg/L)	0.044 \pm 0.011	1.290 \pm 0.335	0.070 \pm 0.037
Dissolved fluoride (mg/L F)	0.273 \pm 0.004	0.214 \pm 0.128	0.408 \pm 0.042
Dissolved chloride (mg/L Cl)	21.588 \pm 2.581	212.539 \pm 83.756	182.944 \pm 22.267
Dissolved ammonium (mg/L NH ₄)	0.159 \pm 0.363	13.500 \pm 3.122	0.032 \pm 0.023
Dissolved nitrite (mg/L NO ₂)	0.060 \pm 0.068	0.000 \pm 0.000	0.000 \pm 0.000
Dissolved nitrate (mg/L NO ₃)	1.572 \pm 0.563	0.154 \pm 0.065	0.156 \pm 0.012
Total dissolved nitrogen (mg/L N)	1.018 \pm 0.196	12.887 \pm 2.806	1.472 \pm 0.321
Dissolved sulphate (mg/L SO ₄)	22.237 \pm 0.926	22.847 \pm 4.922	23.336 \pm 4.667
Dissolved organic carbon (mg/L)	2.734 \pm 0.198	9.296 \pm 2.528	13.008 \pm 0.606
Optical data			
Chlorophyll- α (QSU)	13.498 \pm 0.878	23.554 \pm 2.673	112.907 \pm 49.080
Peak T (QSU)	11.163 \pm 1.250	216.009 \pm 73.926	345.900 \pm 232.760
Peak C (QSU)	11.983 \pm 1.577	134.818 \pm 51.430	94.745 \pm 12.658
Absorbance	0.174 \pm 0.028	0.333 \pm 0.077	0.908 \pm 0.351
Turbidity (FNU)	94.361 \pm 11.164	50.133 \pm 7.973	219.347 \pm 201.200

2.4. Data analysis

The statistical significance of variation between water quality parameters for the three different urban water types was obtained using a one-way ANOVA. Linear regression was also used to identify and characterise the relationships between the water quality parameters. The R² value was used to determine the strength of the correlation, as well as to determine the significance ($p < 0.05$). All statistics were performed in Prism 9 (GraphPad, CA, USA).

3. Results

3.1. Water quality within Kolkata city

Average values of key physicochemical and chemical water quality parameters, for the different water types (Hooghly River, Canals and EKW), are shown in Table 1, as well as the optical data obtained from the VLux TPro sensor deployment.

The physicochemical data shown in Table 1 demonstrates the diversity of the water bodies studied. The canal waters exhibit properties that are characteristic of waters impacted by untreated sewage wastewater, with very low dissolved oxygen (DO) concentrations in comparison to the Hooghly River, alongside high conductivity values, phosphorus (both soluble reactive phosphorus and total phosphorus), dissolved ammonium and dissolved organic carbon (DOC) concentrations (Table 1). One-way ANOVA analyses for all these parameters demonstrate significant differences ($p < 0.05$) for all these parameters between the different water types. The canal and EKW waters also demonstrate high chloride concentrations while all three water types contain <0.5 mg/L of fluoride (Table 1), comparable with other natural freshwaters (Chilton et al., 2006). The EKW exhibits the highest pH, DO and DOC values, but significantly lower phosphorus and dissolved ammonium concentrations ($p < 0.05$) than those observed in the canal and Hooghly River waters which feed this wetland system (Table 1). The dissolved sulphate concentrations are consistent across the different waters assessed, with no significant differences between the waters identified.

The VLux TPro sensor data, shown in Table 1, also shows that the canal and EKW waters exhibit significantly higher Peak T (tryptophan-like fluorescence, TLF, $\lambda_{ex}/\lambda_{em}$ 280/365 (± 25) nm), and Peak C fluorescence (associated with humic-like natural organic matter, $\lambda_{ex}/\lambda_{em}$ 280/450 (± 25) nm), by an order of magnitude, than the Hooghly River

($p < 0.05$). Surprisingly, this difference in water quality of the three water types is not clearly identified within the turbidity data ($p > 0.05$), largely due to the high variability of the turbidity within and between the water body types. The EKW waters also demonstrate chlorophyll- α fluorescence intensity that is an order of magnitude greater than that of the other urban water bodies assessed here, with a one-way ANOVA identifying significant differences ($p < 0.05$) identified between the chlorophyll- α intensity for each water type.

Correlations between Peak T fluorescence and the physicochemical and chemical data were explored using linear regression. Significant, albeit weak, correlations were identified between Peak T fluorescence and conductivity ($R^2 = 0.34$, $p < 0.05$), and dissolved nitrate concentrations ($R^2 = 0.39$, $p < 0.05$). A strong significant relationship was identified between Peak T and DOC ($R^2 = 0.74$, $p < 0.001$). Peak T fluorescence did not demonstrate significant linear relationships ($p > 0.05$) with any of the

other field physicochemical parameters or chemical data when assessing all water types combined.

3.1.1. Biological water quality within Kolkata city

The biological enumeration data highlights the heavy biological contamination within the canal waters, with these waters demonstrating the highest *E. coli* and coliforms counts of the three water types (Fig. 2a). The total bacterial cell counts demonstrate the high levels of bacteria in the canals, but also in the EKW (Fig. 2b). However, this data does not determine the species or viability of the cells present.

A moderate significant correlation, determined using linear regression, was identified between Peak T fluorescence intensity and the total bacteria cell count across all samples ($R^2 = 0.51$, $p < 0.01$). No significant correlations were identified between Peak T and *E. coli* or coliform enumeration ($p > 0.05$) for all water types.

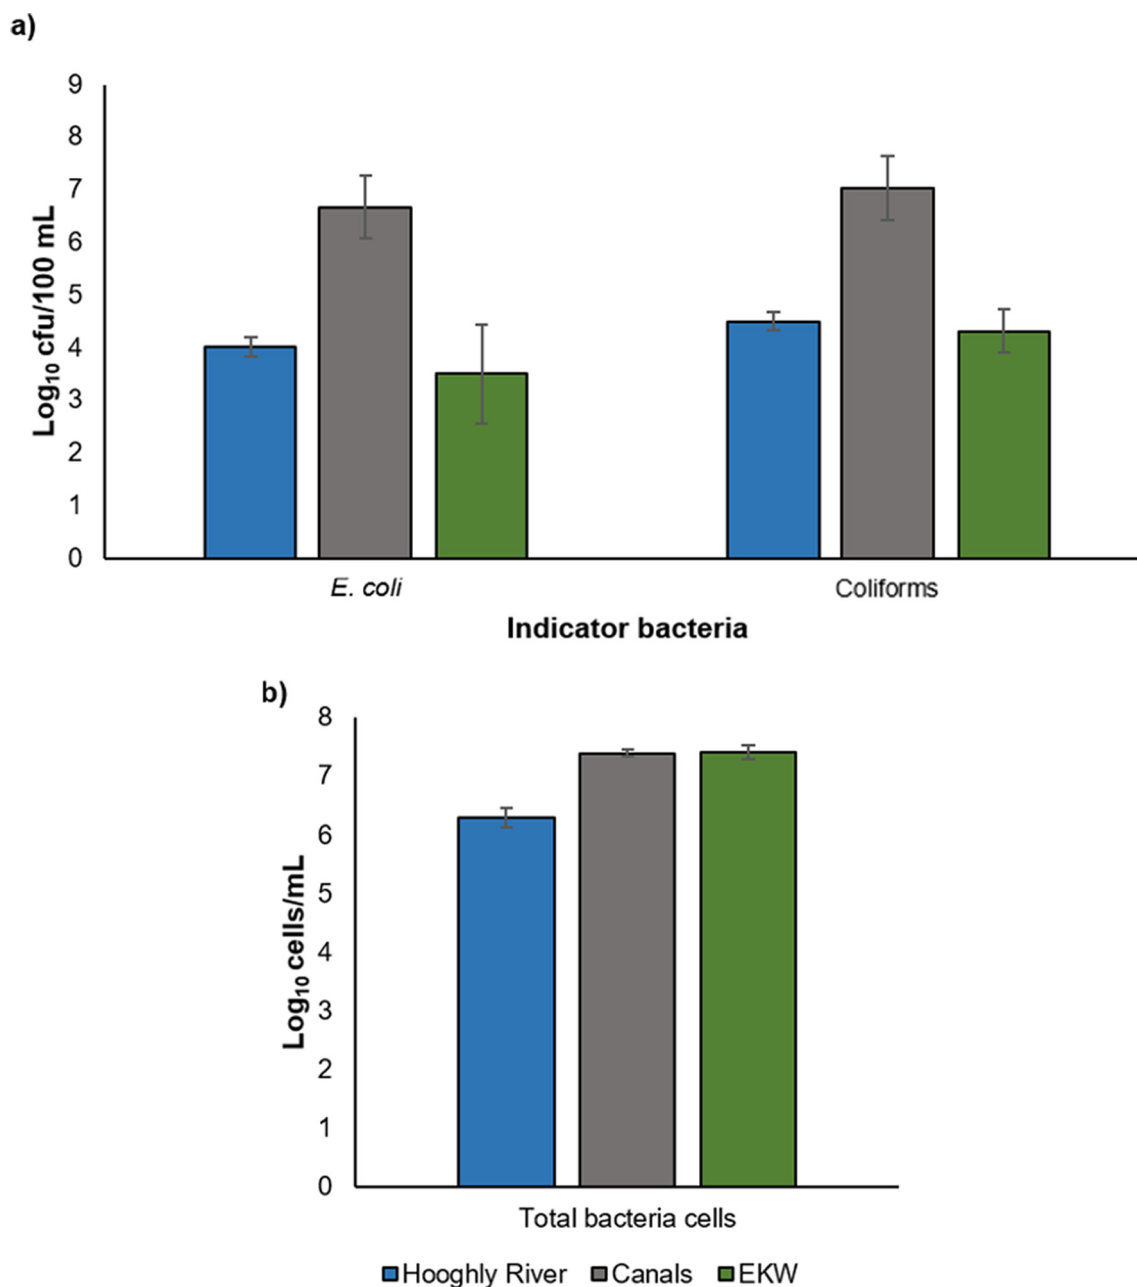


Fig. 2. Average bacterial enumeration data (\pm SD) for the three urban water types; Hooghly River (blue), canals (grey) and East Kolkata Wetlands (green): a) *E. coli* and coliform enumeration data (\log_{10} cfu/100 mL); b) total bacteria cells (\log_{10} cells/mL). Data shown is the parameter average for each water type with error bars representing ± 1 standard deviation: six field sites on the Hooghly River; four canal water field sites; and two field sites in the East Kolkata Wetlands (EKW).

3.2. The identification of a contamination event

The VLux TPro sensor was deployed in the Hooghly River to assess the ability of the sensor to identify bacterial pollution events in a complex surface water. Fig. 3 shows the VLux TPro data from a boat study which was conducted across six sampling sites, on a 3 km stretch of the Hooghly River, over a two-hour monitoring period; the study site map is shown in the Section 2.2 (Fig. 1).

From this data, a contamination event can clearly be identified at sampling location H5, where there was a visually fast-flowing wastewater drain (almost 4 m wide) approximately 50 m upstream of the sampling point. This contamination event at site H5 is easily seen in the VLux TPro Peak T data (Fig. 3a), which shows almost an order of magnitude increase (98.67 ± 1.25 QSU) in comparison to upstream sampling sites H1-H4

(9.77–12.71 QSU). This is also reflected, to a lesser extent, in the Peak C data which demonstrates almost a fourfold increase in intensity from 11.98 to 13.85 QSU upstream to 42.35 ± 0.78 QSU at H5. The VLux TPro absorbance data also reflects the contamination event, demonstrating a doubling from the upstream sampling locations (Fig. 3b). However, this event is not clearly identified by the turbidity data, with comparable elevated turbidity at sites H4 and H5 (Fig. 3b).

Fig. 4 shows physicochemical, chemical and microbiological data for the samples collected from the Hooghly River boat survey. The contamination event at sampling location H5 is identifiable from the physicochemical and chemical data at H5 compared to the upstream sampling locations (H1-H4): increases, by two orders of magnitude, in total phosphorus (from 0.031 to 0.062 mg/L upstream to 0.656 mg/L at H5) and dissolved ammonium concentration (from 0.008 to 0.015 mg/L upstream to 3.3 mg/L at

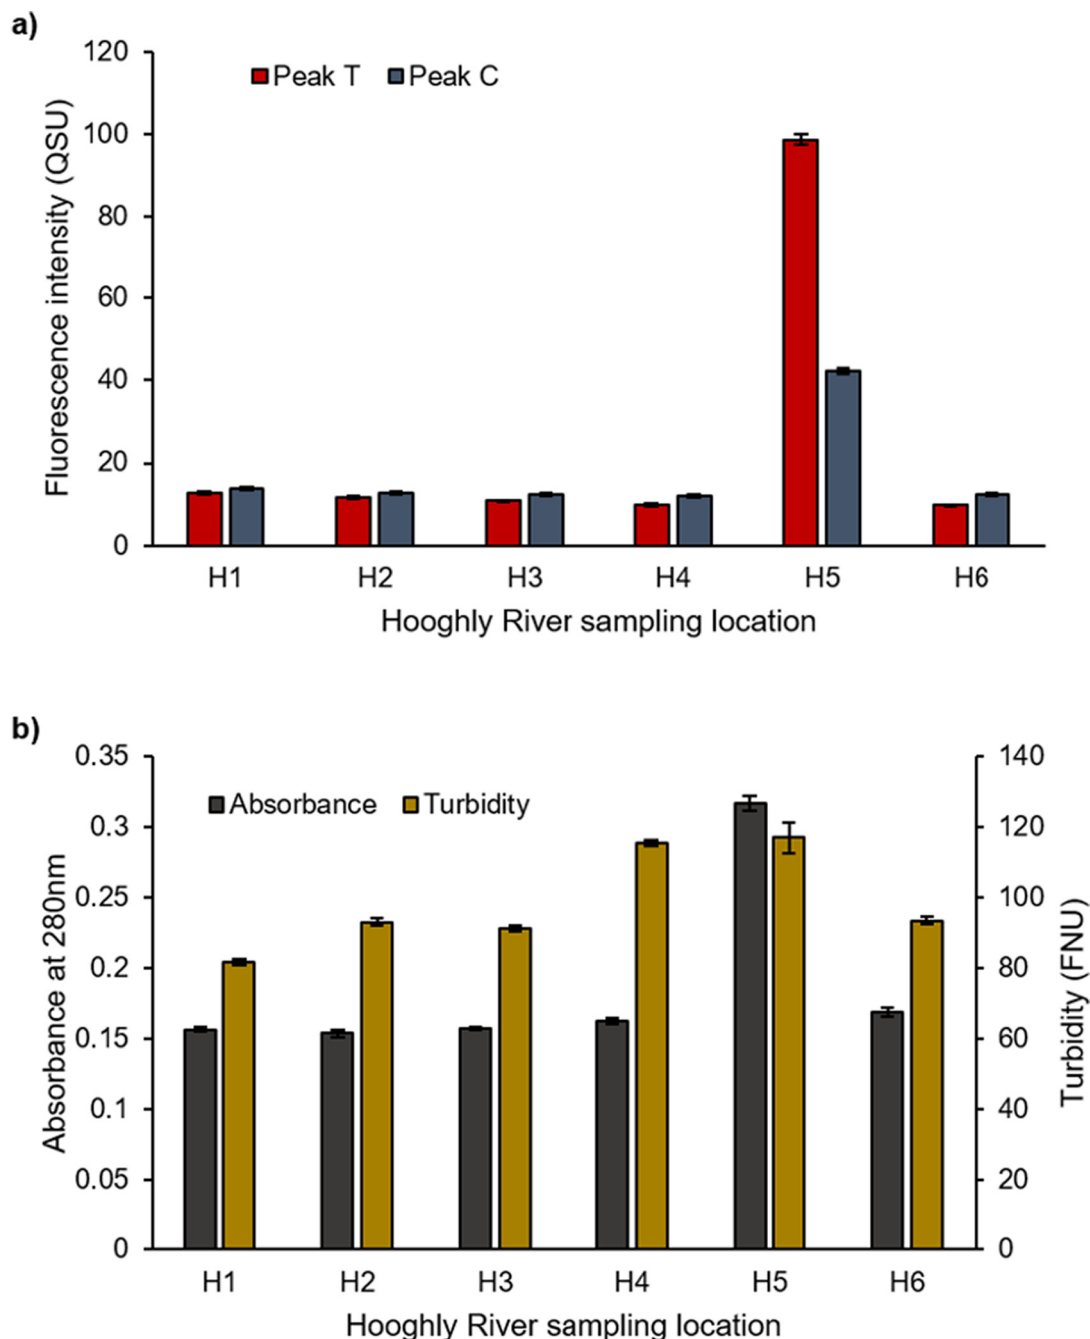


Fig. 3. VLux TPro fluorescence data for the Hooghly River boat sampling survey, demonstrating a biological contamination event (from an urban drain) at sampling location H5: a) Peak T fluorescence intensity (QSU); b) Peak C fluorescence (QSU). Data is averaged over a minute of sampling ($n = 60$), error bars represent ± 1 standard deviation.

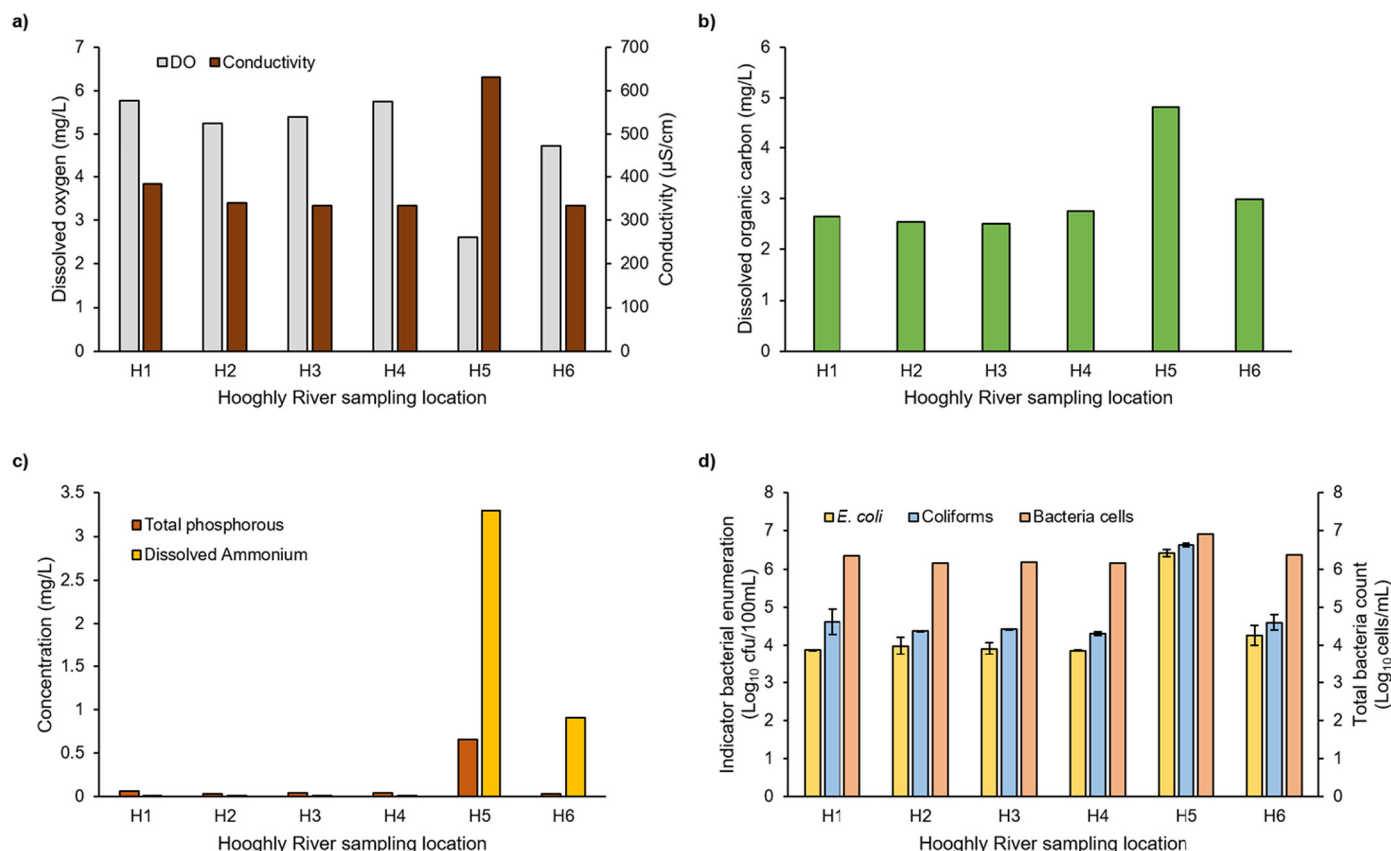


Fig. 4. Hooghly River data demonstrating a biological contamination event (from an urban drain) at H5: a) Concentration of total phosphorus (mg/L) and dissolved ammonium (mg/L); b) Dissolved organic carbon (DOC) concentration (mg/L); c) Field conductivity ($\mu\text{S}/\text{cm}$) and dissolved oxygen (mg/L) data; d) bacterial enumeration data for *E. coli* and coliforms (Log_{10} cfu/100 mL), replicated in triplicate ($n = 3$) with error bars representing ± 1 standard deviation, and total bacteria cell counts (Log_{10} cells/mL).

H5); DOC almost doubles from 2.51 to 2.76 mg/L upstream to 4.83 mg/L at H5; the DO concentration halves from 5.26 to 2.61 mg/L at H5; conductivity doubles from 346 to 664 $\mu\text{S}/\text{cm}$ at H5; at least a two-log increase in bacterial enumeration is seen from 4.63×10^3 - 2.79×10^4 *E. coli* Log_{10} cfu/100 mL upstream to 3.07×10^6 *E. coli* Log_{10} cfu/100 mL, and 4.24×10^4 - 4.35×10^5 coliforms (cfu/mL) upstream to 1.15×10^7 coliforms (Log_{10} cfu/100 mL) at H5; and an increase in total bacteria cell counts is also seen at H5. This is indicative of pollution from a raw sewage source.

When analysing the data for the Hooghly River only, strong significant correlations ($R^2 \geq 0.85$, $p < 0.01$) were seen between Peak T fluorescence intensity and many of the physicochemical and chemical parameters measured (Figs. 3 and 4). Total phosphorus and soluble reactive phosphorus demonstrated very significant strong correlations with Peak T ($R^2 = 0.999$, $p < 0.0001$), as well as dissolved ammonium also demonstrating a strong positive correlation ($R^2 = 0.92$, $p < 0.001$), as shown by Fig. 3a. DOC concentrations (Fig. 4b) also correlated strongly with Peak T fluorescence ($R^2 = 0.94$, $p < 0.001$), with a weaker linear relationship between Peak C and DOC ($R^2 = 0.90$, $p < 0.01$). DO and conductivity also demonstrate strong significant linear correlations with Peak T fluorescence, $R^2 = 0.89$ ($p < 0.01$) and $R^2 = 0.98$ ($p < 0.0001$) respectively. Strong significant correlations between Peak T and bacterial enumeration data, *E. coli*, coliforms and total bacteria cell counts, are seen for the Hooghly River samples; $R^2 = 0.999$, $p < 0.0001$, $R^2 = 0.999$, $p < 0.0001$ and $R^2 = 0.91$, $p < 0.001$ respectively.

A more limited study was also undertaken in the post-monsoon season (December 2019); field locations shown in Supplementary Fig. 1 and detailed in Supplementary Table 2, with summary data presented in Supplementary Table 3. Initial observations show little differences in the sensor data, with some seasonal variation in the physicochemical parameters.

Further work to map this over space and time, and to further assess the potential application of Peak T as a novel water quality parameter, is needed.

4. Discussion

Single channel *in situ* fluorescence sensors have been used in freshwater systems to assess the quality of urban surface freshwaters (Khamis et al., 2017; Mendoza et al., 2020). However, these studies have been limited by optical interferences and the inability to collect quantitative fluorescence data, related to unit standardisation. This study presents the first freshwater field deployment of a multichannel *in situ* fluorescence sensor which provides internally corrected fluorescence data in standard units (QSU). The sensor deployment occurred as part of a sampling survey, conducted in March 2019, of different urban waters within Kolkata, India. By monitoring physicochemical, chemical and biological water quality parameters alongside the VLux TPro sensor, this study has been able to obtain a truly quantitative Peak T data set. This data sets provides the ability to evaluate the relationship of *in situ* Peak T data with a suite of field and laboratory water quality parameters, and assess the benefit of using fluorescence within water quality and water management.

4.1. Water quality of the Hooghly River within Kolkata city

The Hooghly River at Kolkata is classified by the Central Pollution Control Board of India as Class D (heavily polluted), although it's designated as Class B (slight pollution); where waters are designated for use for organised outdoor bathing (Central Pollution Control Board, 2013; National River Conservation Directorate, 2009). The pH and DO data for the Hooghly River in this study, shown in Table 1, demonstrates compliance with the water quality standards for Class B waters, where the pH

must be between 6.5 and 8.5 and the DO >5 mg/L waters (Central Pollution Control Board, 2013; National River Conservation Directorate, 2009), which aligns with others studies (National River Conservation Directorate, 2009) and the post-monsoon survey conducted in December 2019 (Supplementary Table 3). However, the Hooghly River in Kolkata fails to meet the Class B criteria for Biochemical Oxygen Demand (BOD), <3 mg/L, and total coliforms, <500 most probable number (MPN)/100 mL (National River Conservation Directorate, 2009). This failure was also seen in the bacterial enumeration in this study where the total coliforms (combined *E. coli* and coliform counts) are more than two-log higher (Fig. 2) than permitted maximum enumeration (2500 MPN/100 mL), but in agreement with other monitoring data for this stretch of the Hooghly River (Central Pollution Control Board, 2013). It is these biological failures that cause the water quality status of the Hooghly River in Kolkata to be classified as Class D (Table 1) (National River Conservation Directorate, 2009). Conversely, the biological water quality status of this section of the river is classified as Class C (moderately polluted) (Bio-Science Division and Central Pollution Control Board, 2018; Central Pollution Control Board, 2017). This is based on the saprobic and diversity scores of macro-invertebrate benthic fauna (Bio-Science Division and Central Pollution Control Board, 2018).

4.2. Peak T: a new water quality parameter

Many physicochemical and chemical water quality parameters can now be monitored *in situ* using real-time sensors and report data remotely via telemetry systems. At present, both microbiological and biological water quality monitoring requires time consuming discrete sampling surveys, yet it is evident from the data in this study, and others (Central Pollution Control Board, 2013; National River Conservation Directorate, 2009), that biological water quality is essential for determining the aquatic ecosystem health and long-term effects of pollutants (Bio-Science Division and Central Pollution Control Board, 2018; Central Pollution Control Board, 2017). The use of Peak T fluorescence has, until now, been hindered by technological issues, such as how to account for optical interferences (Khamis et al., 2017; Mendoza et al., 2020), as well as understanding what water quality criteria Peak T relates to. With technological advances and improved scientific knowledge, the use of *in situ* Peak T fluorescence could provide information regarding biological activity and underpinning system health.

Previously, Peak T has been correlated with faecal indicator species, such as *E. coli*, leading to the notion that Peak T fluorescence could act as a proxy for bacterial indicator species counts (Carstea et al., 2020; Sorensen et al., 2018b; Sorensen et al., 2018a; Sorensen et al., 2016; Sorensen et al., 2015a). Significant correlations between Peak T fluorescence intensity and *E. coli* or coliform enumeration were not identified across all water types in this study. However, a significant correlation was seen between Peak T and total bacteria cell count ($R^2 = 0.51$, $p < 0.01$). This indicates that Peak T fluorescence, a ubiquitous fluorescence signature across multiple bacterial species (Elliott et al., 2006; Fox et al., 2017; Goto et al., 2020), could be used to provide information regarding the overall microbial community activity and metabolism, rather than being species specific, particularly in varying and complex water matrices (Fox et al., 2019; Fox et al., 2017; Goto et al., 2017; Lønborg et al., 2009; Paerl et al., 2003; Romera-Castillo et al., 2011). When analysing the Hooghly River data only, very strong significant correlations between Peak T and the microbiological data are identified ($R^2 \geq 0.91$, $p < 0.001$). This suggests that grouping water types and understanding system baseline values and fluctuations can enhance the benefit of Peak T fluorescence for water quality monitoring, but that there is still value in this parameter without having this prior knowledge.

Peak T fluorescence is again seen to show few significant correlations with the chemical data across all samples, with DOC demonstrating the only strong correlation with Peak T ($R^2 = 0.74$, $p < 0.001$). Similar relationships between DOC and Peak T fluorescence have been reported previously, with Peak T being associated with the labile DOC fraction (Carstea

et al., 2020; Coble et al., 1993; Judd et al., 2006; Yang et al., 2014). Surprisingly, no significant correlation is identified between Peak T and DO, a physicochemical water quality parameter that has long been associated with Peak T due to the use of DO, and the biochemical oxygen demand (BOD), to infer biological activity levels (Ahmad and Reynolds, 1999; Baker and Inverarity, 2004; Hudson et al., 2008; Khamis et al., 2021; Reynolds and Ahmad, 1997; Yang et al., 2014). No significant correlation between Peak T and turbidity is observed. Previous research has reported the use of turbidity measurements as an indicator of bacterial contamination (Jung et al., 2014). However the presence of high sediment and pollution loading within complex surface waters (Allen et al., 2008), such as the Hooghly River, means that turbidity measurements cannot be used as a reliable indicator of bacterial contamination. Peak T data for the Hooghly River does exhibit a strong significant correlation ($R^2 = 0.85$, $p < 0.01$) with the total number of bacterial cells (determined by flow cytometry). This suggests that Peak T provides a potential insight into microbial activity within freshwater ecosystems, encompassing many frequently measured parameters and, therefore, providing a clear benefit for using this *in situ* and real-time parameter for high spatio-temporal resolution water quality monitoring.

Comparing Peak T to standard water chemistry can be useful for exploring the relationship of Peak T fluorescence with other water quality parameters. However, this study demonstrates that Peak T fluorescence data is best used independently to other water quality parameters as it can provide information that directly relates to the microbiological activity within the aquatic system under investigation. At present such information cannot be provided by current monitoring parameters. None of the physicochemical or biological data collected as part of time constrained discrete sampling surveys provide insight into the daily real-time activity of the aquatic microbial community. It is also clear from the data here that Peak T fluorescence can be utilised to identify contamination events or microbial activity in complex water matrices. As such, deploying the VLux TPro sensor could greatly improve the monitoring of biological contamination hotspots and point-source pollution from sewage inputs into river systems. Through improved resolution of water quality measurements through time and space, both quality and resources can be better managed.

4.3. Using Peak T fluorescence *in situ* to identify contamination events

This study uses *in situ* Peak T fluorescence to identify pollution events in the Hooghly River, within the densely populated urban area of Kolkata. A pollution event is clearly identified within the quantitative Peak T data, obtained from the VLux TPro sensor, as shown by Fig. 3a. The contamination event at sampling site H5 is easily identified from the background Peak T fluorescence, without the need for prior knowledge of the baseline and diurnal or seasonal variations. This contamination event is also identified within the other water quality parameters monitored here (Figs. 3 and 4), obtained during the field survey or from laboratory analysis of collected water samples. This data suggests the pollution is likely to be derived from a raw sewage source. Whilst many of the physicochemical and chemical water quality parameters measured can be monitored *in situ*, a suite of sensors would be required to obtain information which can allow the diagnosis of contamination. This can be extremely costly, hindering the uptake of such multiparameter *in situ* monitoring and limiting the spatio-temporal resolution of the data collected. Ultimately, this reduces the identification of contamination events and prevents improved monitoring and management of water quality. *In situ* Peak T fluorescence provides a tool for us to monitor and identify contamination hotspots more readily than current practices, and could provide an insight into ecosystem health, *via* microbial activity, which would otherwise only be available by adopting a multiparameter approach.

Although further work is required to determine the true implications of this, such a water quality parameter could be of great benefit for water quality management. This highlights the benefit of *in situ* real-time Peak T fluorescence for the identification of a range of pollution sources and events.

4.4. Potential application of the VLux TPro sensor and future work

By understanding the signatures of different water types monitored in this study (Table 1), the contamination event at sampling location H5 can be identified as wastewater contamination (Figs. 3 and 4). This highlights the benefit of detailed and in-depth analysis for monitoring contamination events. However, such a comprehensive data set is time consuming, expensive and difficult to obtain with good spatio-temporal resolution. The transient nature of the contamination event demonstrates the difficulty in monitoring such large systems via discrete sampling only. To improve the identification of such contamination events, the VLux TPro could be deployed on the 57 existing water quality monitoring stations on the Ganges/Hooghly system, 10 of which are within the state of West Bengal and 2 are within Kolkata (Central Pollution Control Board, 2013). Alternatively, these robust sensors could be deployed on shipping or passenger boats. This would greatly improve spatio-temporal resolution of water quality monitoring and further explore locations of frequent contamination.

Further exploratory work is required to assess the application of the VLux TPro, and to assess the ability of this novel fluorimeter to perform, as reported here, in different systems and to assess the impact of seasonality on sensor application. A limited study using the VLux TPro was also undertaken within Kolkata in the post-monsoon season (December 2019). Initial observations show little differences in the sensor data, with some seasonal variation in the physicochemical parameters. However, further deployments to assess both spatial and temporal variations are required to provide a more detailed understanding of the application of Peak T as a novel water quality parameter.

In addition, fluorescence characterisation of different industrial effluents, which are known to add to the pollution of the Hooghly River, should be assessed to provide added benefit to the inclusion of such multi-channel fluorimeters into regular water quality monitoring. This would aid tracing of pollution events and origins within freshwater systems, enabling more effective management of pollution sources.

The data derived from the EKW waters demonstrates effective nutrient sequestration within the wetland system, when compared to the canal waters which feed this wetland system (Table 1). Interpreting the EKW data is limited by the number of sample sites of 'clean' waters in this system. Further work on wetland systems, and the relationship of Peak T and chlorophyll- α with algal populations, is needed to fully explore the potential of the VLux TPro sensor for monitoring eutrophic waters. However, monitoring the EKW system does allow us to understand how we may be able to identify highly eutrophic inputs to the main river system, perhaps from tributaries or eutrophication events related to land use practices.

5. Conclusions

- This study provides the first *in situ* fluorescence case study of its kind using a sensor with in-built corrections for turbidity and absorbance, reporting fluorescence data quantitatively in standardised units, QSU. These technological advances allow Peak T fluorescence data to be collected and compare a range of urban waters systems.
- Peak T fluorescence provides *in situ* information regarding biological water quality, biological contamination events and microbial activity, something previously limited to time consuming and expensive discrete sampling surveys.
- Peak T fluorescence can identify wastewater contamination in real-time, within a polluted and complex urban surface water matrix.

CRedit authorship contribution statement

Bethany Fox: Conceptualization, Methodology, Software, Formal analysis, Investigation, Data Curation, Writing – Original Draft, Visualization, Project administration.

Robin Thorn: Conceptualization, Methodology, Resources, Writing – Review & Editing, Supervision, Funding acquisition.

Michael Bowes: Investigation, Resources, Data Curation, Writing – Review & Editing.

Daniel Read: Investigation, Resources, Data Curation, Writing – Review & Editing.

Tapan Dutta: Conceptualization, Resources, Writing – Review & Editing, Supervision, Funding acquisition.

Darren Reynolds: Conceptualization, Resources, Writing – Review & Editing, Supervision, Project administration, Funding acquisition.

Funding

This study was funded by the Natural Environment Research Council, UK [NE/R003106/1] and Department of Science and Technology, India [DST/TM/INDO-UK/2K17/30].

Data availability

The data required to reproduce the above findings are available to download from <https://doi.org/10.5285/9bc3dce7-7c2b-49dd-9b76-819267d7a352> (Fox et al., 2022).

Declaration of competing interest

The authors declare that they have no known competing financial interests or personal relationships that could have appeared to influence the work reported in this paper.

Acknowledgments

The authors would like to thank the team at Bose Institute, Kolkata, for facilitating the sampling surveys and laboratory work in Kolkata. The authors would also like to acknowledge Chelsea Technologies Ltd. for ongoing VLux TPro sensor support, as well as UKCEH for conducting additional sample analysis.

Appendix A. Supplementary material

Supplementary data to this article can be found online at <https://doi.org/10.1016/j.scitotenv.2022.156848>.

References

- Aazami, J., Esmaili-Sari, A., Abdoli, A., Sohrabi, H., Van Den Brink, P.J., 2015. Monitoring and assessment of water health quality in the Tajan River, Iran using physicochemical, fish and macroinvertebrates indices. *J. Environ. Health Sci. Eng.* 13, 1–12. <https://doi.org/10.1186/s40201-015-0186-y>.
- Ahmad, S.R., Reynolds, D.M., 1999. Monitoring of water quality using fluorescence technique: prospect of on-line process control. *Water Res.* 33, 2069–2074. [https://doi.org/10.1016/S0043-1354\(98\)00435-7](https://doi.org/10.1016/S0043-1354(98)00435-7).
- Allen, M., Brecher, R., Copes, R., Hrudehy, S., Payment, P., 2008. *Turbidity and Microbial Risk in Drinking Water*.
- Baker, A., Inverarity, R., 2004. Protein-like fluorescence intensity as a possible tool for determining river water quality. *Hydrol. Process.* 18, 2927–2945. <https://doi.org/10.1002/hyp.5597>.
- Bhattacharjee, C., 2014. Canals and its relevance to the Kolkata Megacity. *Abhinav Natl. Mon. Ref. J. Res. Arts Educ.* 3, 20–24.
- Bio-Science Division, Central Pollution Control Board, 2018. *Biological Water Quality Assessment of the River Ganga (2017-18)*.
- Blaen, P.J., Khamis, K., Lloyd, C.E.M., Bradley, C., Hannah, D., Krause, S., 2016. Real-time monitoring of nutrients and dissolved organic matter in rivers: capturing event dynamics, technological opportunities and future directions. *Sci. Total Environ.* 569–570, 647–660. <https://doi.org/10.1016/j.scitotenv.2016.06.116>.
- Bowes, M.J., Read, D.S., Joshi, H., Sinha, R., Ansari, A., Hazra, M., Simon, M., Vishwakarma, R., Armstrong, L.K., Nicholls, D.J.E., Wickham, H.D., Ward, J., Carvalho, L.R., Rees, H.G., 2020. Nutrient and microbial water quality of the upper Ganga River, India: identification of pollution sources. *Environ. Monit. Assess.* 192. <https://doi.org/10.1007/s10661-020-08456-2>.
- Carstea, E.M., Popa, C.L., Baker, A., Bridgeman, J., 2020. In situ fluorescence measurements of dissolved organic matter: a review. *Sci. Total Environ.* 699, 134361. <https://doi.org/10.1016/j.scitotenv.2019.134361>.
- Central Pollution Control Board, 2020. *Guidelines for Setting up of Biodiversity Parks in Floodplains of Rivers of India, Including River Ganga*.

- Central Pollution Control Board, 2017. *Biological Indicators of Water Quality in River Ganga*. Central Pollution Control Board, 2013. *Pollution Assessment: River Ganga*.
- Chilton, J., Dahi, E., Lennon, M., Jackson, P., 2006. *Fluoride in Drinking-water*.
- Chowdury, M.S.U., Emran, T.B., Ghosh, S., Pathak, A., Alam, M.M., Absar, N., Andersson, K., Hossain, M.S., 2019. IoT based real-time river water quality monitoring system. *Procedia Comput. Sci.* 155, 161–168. <https://doi.org/10.1016/j.procs.2019.08.025>.
- Coble, P.G., Lead, J., Baker, A., Reynolds, D.M., Spencer, R.G.M., 2014. *Aquatic Organic Matter Fluorescence*. Cambridge University Press.
- Coble, P.G., Schultz, C.A., Mopper, K., 1993. Fluorescence contouring analysis of DOC intercalibration experiment samples: a comparison of techniques. *Mar. Chem.* 41, 173–178. [https://doi.org/10.1016/0304-4203\(93\)90116-6](https://doi.org/10.1016/0304-4203(93)90116-6).
- Cyr, F., Tedetti, M., Besson, F., Bhairy, N., Goutx, M., 2019. A glider-compatible optical sensor for the detection of polycyclic aromatic hydrocarbons in the marine environment. *Front. Mar. Sci.* 6, 1–15. <https://doi.org/10.3389/fmars.2019.00110>.
- East Kolkata Wetlands Management Authority, 2019. *East Kolkata Wetlands Management Authority Home Page [WWW Document]*.
- EKWMA, 2016. *East Kolkata Wetlands Management Authority (EKWMA) Report 2013-2014 to 2015-2016*.
- Elliott, S., Lead, J.R., Baker, A., 2006. Characterisation of the fluorescence from freshwater, planktonic bacteria. *Water Res.* 40, 2075–2083. <https://doi.org/10.1016/j.watres.2006.03.017>.
- Firth, P., 1999. *The importance of water resources education for the next century*. *J. Am. Water Resour. Assoc.* 35, 487–492.
- Fox, B.G., 2018. *Bacterial processing of fluorescent organic matter in freshwater*. Retrieve from University of the West of England. <https://uwe-repository.worktribe.com/output/863820>.
- Fox, B.G., Thom, R.M.S., Anesio, A.M., Cox, T., Attridge, J.W., Reynolds, D.M., 2019. Microbial processing and production of aquatic fluorescent organic matter in a model freshwater system. *Water* 11. <https://doi.org/10.3390/w11010010>.
- Fox, B.G., Thom, R.M.S., Anesio, A.M., Reynolds, D.M., 2017. The in situ bacterial production of fluorescent organic matter; an investigation at a species level. *Water Res.* 125, 350–359. <https://doi.org/10.1016/j.watres.2017.08.040>.
- Fox, B.G., Thom, R.M.S., Dutta, T.K., Reynolds, D.M., 2022. *Water Quality of Urban Surface Freshwater in Kolkata, India, June 2018 to December 2019*. <https://doi.org/10.5285/9bc3dce7-7c2b-49dd-9b76-819267d7a352>.
- Gangopadhyay, A., Patra, P., 2019. The historical background of the canal system in Calcutta, India, and its contribution to development. *Proc. Inst. Civ. Eng. - Eng. Hist. Herit.* 173, 80–91. <https://doi.org/10.1680/jenh.19.00024>.
- Gangopadhyay, S.G., Gupta, J., 2008. *Rejuvenating the Kestopur canal system in the Kolkata Metropolitan Area*. *Itpi J.* 5, 47–54.
- Goto, S., Tada, Y., Suzuki, K., Yamashita, Y., 2020. Evaluation of the production of dissolved organic matter by three marine bacterial strains. *Front. Microbiol.* 11, 1–15. <https://doi.org/10.3389/fmicb.2020.584419>.
- Goto, S., Tada, Y., Suzuki, K., Yamashita, Y., 2017. Production and reutilization of fluorescent dissolved organic matter by a marine bacterial strain, *Alteromonas macleodii*. *Front. Microbiol.* 8, 1–10. <https://doi.org/10.3389/fmicb.2017.00507>.
- Hudson, N., Baker, A., Ward, D., Reynolds, D.M., Brunson, C., Carliell-Marquet, C., Browning, S., 2008. Can fluorescence spectrometry be used as a surrogate for the biochemical oxygen demand (BOD) test in water quality assessment? An example from south West England. *Sci. Total Environ.* 391, 149–158. <https://doi.org/10.1016/j.scitotenv.2007.10.054>.
- ISO, 1999. *ISO 7027: 1999(E) Water Quality – Determination of Turbidity*.
- Judd, K.E., Crump, B.C., Kling, G.W., 2006. Variation in dissolved organic matter controls bacterial production and community composition T1 - 87. *Ecology* 87, 2068–2079. [https://doi.org/10.1890/0012-9658\(2006\)87\[2068:VIDOMC\]2.0.CO;2](https://doi.org/10.1890/0012-9658(2006)87[2068:VIDOMC]2.0.CO;2) VN-r.
- Jung, A.V., Cann, P., Le, Roig, B., Thomas, O., Baurès, E., Thomas, M.F., 2014. Microbial contamination detection in water resources: interest of current optical methods, trends and needs in the context of climate change. *Int. J. Environ. Res. Public Health* 11, 4292–4310. <https://doi.org/10.3390/ijerph110404292>.
- Khamis, K., Bradley, C., Gunter, H.J., Basevi, G., Stevens, R., Hannah, D.M., 2021. Calibration of an in-situ fluorescence-based sensor platform for reliable BOD5 measurement in wastewater. *Water Sci. Technol.* 83, 3075–3091. <https://doi.org/10.2166/wst.2021.197>.
- Khamis, K., Bradley, C., Hannah, D.M., 2017. Understanding dissolved organic matter dynamics in urban catchments: insights from in situ fluorescence sensor technology. *Wiley Interdiscip. Rev. Water* 5, e1259. <https://doi.org/10.1002/wat2.1259>.
- Khamis, K., Sorensen, J.P.R., Bradley, C., Hannah, D.M., Lapworth, D.J., Stevens, R., 2015. In situ tryptophan-like fluorometers: assessing turbidity and temperature effects for freshwater applications. *Environ Sci Process Impacts* 17, 740–752. <https://doi.org/10.1039/c5em00030k>.
- Lönborg, C., Álvarez-Salgado, X.A., Davidson, K., Miller, A.E.J., 2009. Production of bioavailable and refractory dissolved organic matter by coastal heterotrophic microbial populations. *Estuar. Coast. Shelf Sci.* 82, 682–688. <https://doi.org/10.1016/j.ecss.2009.02.026>.
- Matilainen, A., Gjessing, E.T., Lahtinen, T., Hed, L., Bhatnagar, A., Sillanpää, M., 2011. An overview of the methods used in the characterisation of natural organic matter (NOM) in relation to drinking water treatment. *Chemosphere* 83, 1431–1442. <https://doi.org/10.1016/j.chemosphere.2011.01.018>.
- Mendoza, L.M., Mladenov, N., Kinoshita, A.M., Pinongcos, F., Verbyla, M.E., Gersberg, R., 2020. Fluorescence-based monitoring of anthropogenic pollutant inputs to an urban stream in Southern California, USA. *Sci. Total Environ.* 718, 137206. <https://doi.org/10.1016/j.scitotenv.2020.137206>.
- National River Conservation Directorate, 2009. *Status Paper on River Ganga: State of Environment and Water Quality Ministry o*, pp. 1–31.
- Paeli, H.W., Dyble, J., Moisaner, P.H., Noble, R.T., Piehler, M.F., Pinckney, J.L., Steppe, T.F., Twomey, L., Valdes, L.M., 2003. Microbial indicators of aquatic ecosystem change: current applications to eutrophication studies. *FEMS Microbiol. Ecol.* 46, 233–246. [https://doi.org/10.1016/S0168-6496\(03\)00200-9](https://doi.org/10.1016/S0168-6496(03)00200-9).
- Patil, P., Sawant, D., Deshmukh, R., 2012. Physico-chemical parameters for testing of water—a review. *Int. J. Environ. Sci.* 3, 1194–1207.
- Peleato, N.M., Legge, R.L., Andrews, R.C., 2017. Investigation of fluorescence methods for rapid detection of municipal wastewater impact on drinking water sources. *Spectrochim. Acta A Mol. Biomol. Spectrosc.* 171, 104–111. <https://doi.org/10.1016/j.saa.2016.07.031>.
- Postel, S., 2015. Water for life. *Front. Ecol. Environ.* 7, 63. <https://doi.org/10.1890/1540-9295-7.2.63>.
- Reynolds, D.M., Ahmad, S.R., 1997. Rapid and direct determination of wastewater BOD values using a fluorescence technique. *Water Res.* 31, 2012–2018. [https://doi.org/10.1016/S0043-1354\(97\)00015-8](https://doi.org/10.1016/S0043-1354(97)00015-8).
- Romera-Castillo, C., Sarmiento, H., Alvarez-Salgado, X.A., Gasol, J.M., Marrasé, C., 2011. Net production and consumption of fluorescent colored dissolved organic matter by natural bacterial assemblages growing on marine phytoplankton exudates. *Appl. Environ. Microbiol.* 77, 7490–7498. <https://doi.org/10.1128/AEM.00200-11>.
- Santos, J.L., Vidal, T., Gonçalves, F.J.M., Castro, B.B., Pereira, J.L., 2021. Challenges to water quality assessment in Europe – is there scope for improvement of the current water framework directive bioassessment scheme in rivers? *Ecol. Indic.* 121. <https://doi.org/10.1016/j.ecolind.2020.107030>.
- Sartory, D.P., Howard, L., 1992. A medium detecting β -glucuronidase for the simultaneous membrane filtration enumeration of *Escherichia coli* and coliforms from drinking water. *Let. Appl. Microbiol.* 15, 273–276. <https://doi.org/10.1111/j.1472-765X.1992.tb00782.x>.
- Sorensen, James P.R., Baker, A., Cumberland, S.A., Lapworth, D.J., MacDonald, A.M., Pedley, S., Taylor, R.G., Ward, J.S.T., 2018. Real-time detection of faecally contaminated drinking water with tryptophan-like fluorescence: defining threshold values. *Sci. Total Environ.* 622–623, 1250–1257. <https://doi.org/10.1016/j.scitotenv.2017.11.162>.
- Sorensen, J.P.R., Lapworth, D.J., Marchant, B.P., Nkhuwa, D.C.W., Pedley, S., Stuart, M.E., Bell, R.A., Chirwa, M., Kabika, J., Liemisa, M., Chibesa, M., 2015a. In situ tryptophan-like fluorescence: a real-time indicator of faecal contamination in drinking water supplies. *Water Res.* 81, 38–46. <https://doi.org/10.1016/j.watres.2015.05.035>.
- Sorensen, J.P.R., Lapworth, D.J., Read, D.S., Nkhuwa, D.C.W., Bell, R.A., Chibesa, M., Chirwa, M., Kabika, J., Liemisa, M., Pedley, S., 2015b. Tracing enteric pathogen contamination in sub-saharan african groundwater. *Sci. Total Environ.* 538, 888–895. <https://doi.org/10.1016/j.scitotenv.2015.08.119>.
- Sorensen, J.P.R., Nayebare, J., Carr, A.F., Lyness, R., Campos, L.C., Ciric, L., Goodall, T., Kulabako, R., Curran, C.M.R., MacDonald, A.M., Owor, M., Read, D.S., Taylor, R.G., 2021. In-situ fluorescence spectroscopy is a more rapid and resilient indicator of faecal contamination risk in drinking water than faecal indicator organisms. *Water Res.* 206, 117734. <https://doi.org/10.1016/j.watres.2021.117734>.
- Sorensen, J.P.R., Sadhu, A., Sampath, G., Sugden, S., Dutta Gupta, S., Lapworth, D.J., Marchant, B.P., Pedley, S., 2016. Are sanitation interventions a threat to drinking water supplies in rural India? An application of tryptophan-like fluorescence. *Water Res.* 88, 923–932. <https://doi.org/10.1016/j.watres.2015.11.006>.
- Sorensen, J.P.R., Vivanco, A., Ascott, M.J., Goody, D.C., Lapworth, D.J., Read, D.S., Rushworth, C.M., Bucknall, J., Herbert, K., Karapanos, I., Gummi, L.P., Taylor, R.G., 2018. Online fluorescence spectroscopy for the real-time evaluation of the microbial quality of drinking water. *Water Res.* <https://doi.org/10.1016/j.watres.2018.03.001>.
- Sutanudjaja, E.H., van Beek, L.P.H., Drost, N., de Graaf, I.E.M., de Jong, K., Peßenteiner, S., Straatsma, M.W., Wada, Y., Wanders, N., Wissler, D., Bierkens, M.F.P., 2018. *PCR-GLOBWB 2.0: a 5 arc-minute global hydrological and water resources model*. *Geosci. Model Dev.* 11, 2429–2453.
- The Environment Agency, 2008. *The Microbiology of Drinking Water (2008) - Part 4 - Methods for the Isolation and Enumeration of Coliform Bacteria Escherichia coli (Including E. coli 0157:H7)*. [https://doi.org/10.1016/S0378-777X\(80\)80046-1](https://doi.org/10.1016/S0378-777X(80)80046-1).
- Yang, L., Shin, H.S., Hur, J., 2014. Estimating the concentration and biodegradability of organic matter in 22 wastewater treatment plants using fluorescence excitation emission matrices and parallel factor analysis. *Sensors* 14, 1771–1786. <https://doi.org/10.3390/s140101771>.
- Zhou, Y., Shi, K., Zhang, Y., Jeppesen, E., Liu, X., Zhou, Q., Wu, H., Tang, X., Zhu, G., 2017. Fluorescence peak integration ratio ICITas a new potential indicator tracing the compositional changes in chromophoric dissolved organic matter. *Sci. Total Environ.* 574, 1588–1598. <https://doi.org/10.1016/j.scitotenv.2016.08.196>.